



**WYATT**  
TECHNOLOGY

6330 Hollister Avenue  
Santa Barbara, CA 93117

Tel: +1 (805) 681-9009  
Fax: +1 (805) 681-0123  
Web: www.wyatt.com

**Pierce BSA**  
**(Lot No: SJ249035)**

## Certificate of Analysis

Pierce Bovine Serum Albumin (BSA)



Wyatt p/n: P8401-02

Lot Number: SJ249035

Manufactured by: Thermo Scientific

Expires: 11/30/2018

Storage: Room Temperature

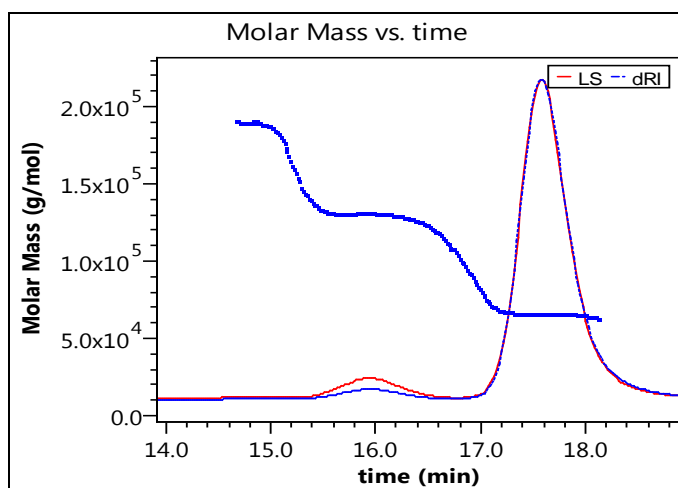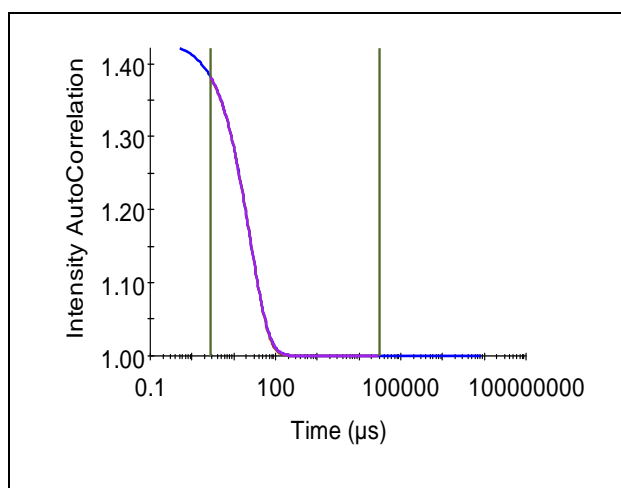

*Standard characterization data by Wyatt DynaPro NanoStar or Plate Reader:*

*Solution filtered through 0.02 µm Anotop filter*

**$R_h$  (from Cumulant) = (3.9 ± 0.1) nm;  $R_h$  (from Regularization) = (4.0 ± 0.3) nm**

*Solution filtered through 0.2 µm Anotop filter*

**$R_h$  (from Cumulant) = (4.3 ± 0.1) nm;  $R_h$  (from Regularization) = (3.9 ± 0.2) nm**

*Standard characterization data by Wyatt MALS detector following SEC separation (WTC-030S5 with PBS at 0.5 mL/min):*

*(Solution filtered through 0.02 µm Anotop filter)*

**Monomer% = 95.3 ± 0.1;  $M_w$  (including aggregates) = (70.0 ± 0.5) kDa**

*(Solution filtered through 0.2 µm Anotop filter)*

**Monomer% = 95.3 ± 0.2 ;  $M_w$  (including aggregates) = (70.8 ± 0.5) kDa**

Certification: Michelle Chen

Date: 11/30/2017